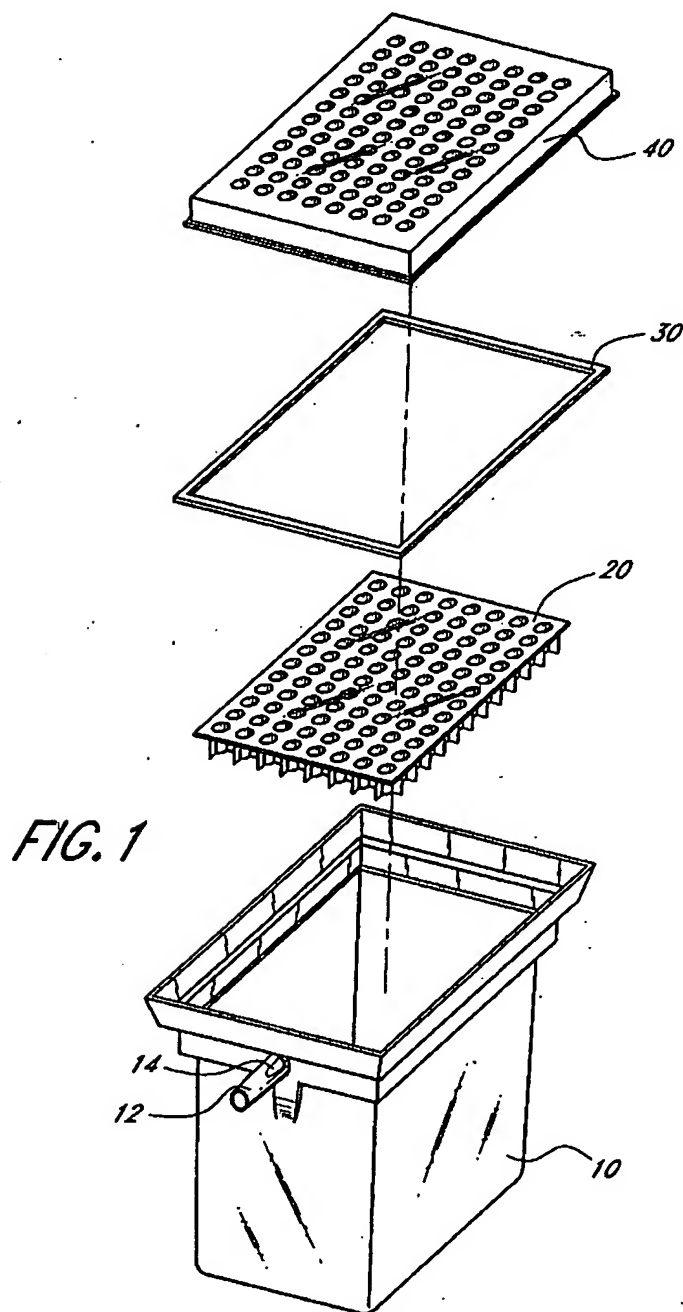
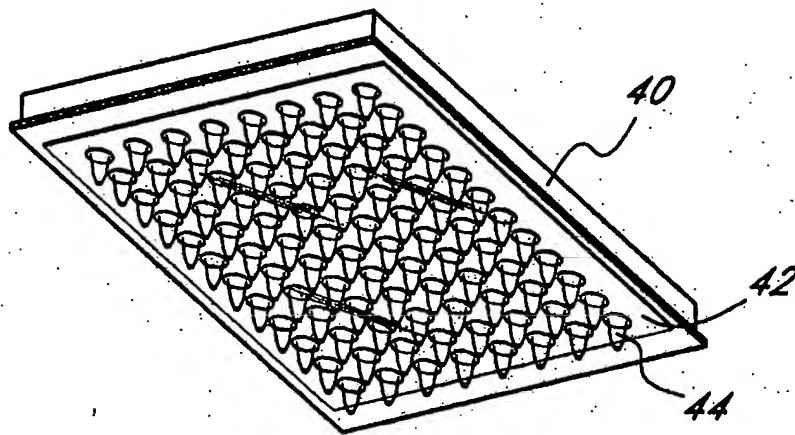


DEVICE AND METHOD FOR HIGH-THROUGHPUT  
QUANTIFICATION OF MRNA FROM WHOLE BLOOD

Masato Mitsuhashi

Appl. No.: Unknown Atty Docket: HITACHI.055CP1





*FIG. 2*


DEVICE AND METHOD FOR HIGH-THROUGHPUT  
QUANTIFICATION OF MRNA FROM WHOLE BLOOD

Masato Mitsuhashi

Appl. No.: Unknown


Atty Docket: HITACHI.055CP1

FIG 3.

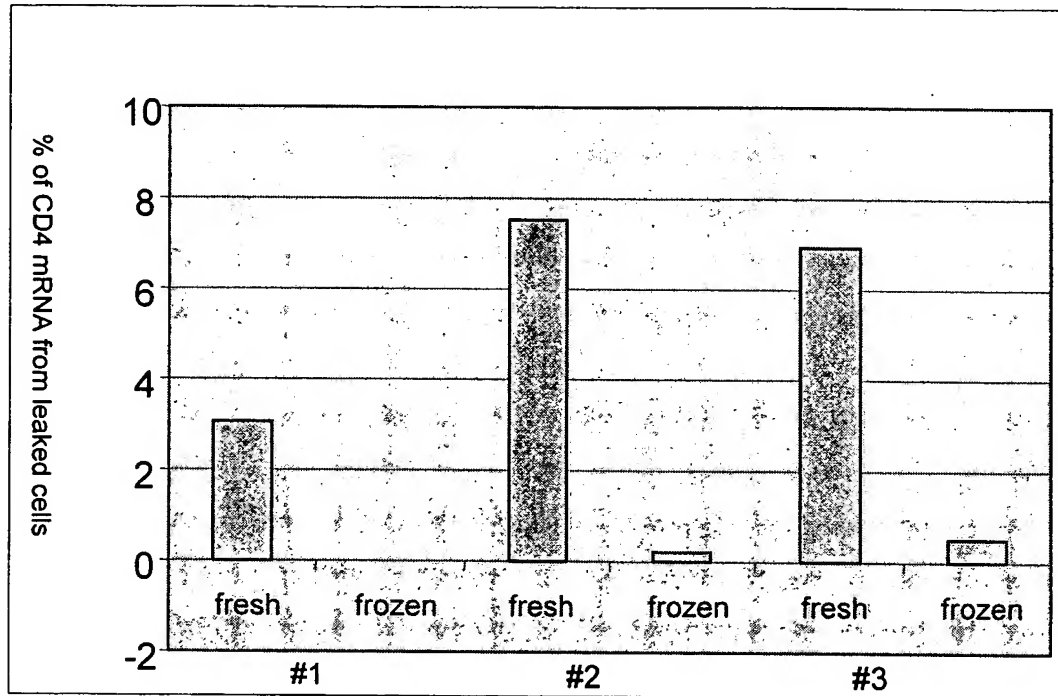


BEST AVAILABLE COPY

FIG 4.

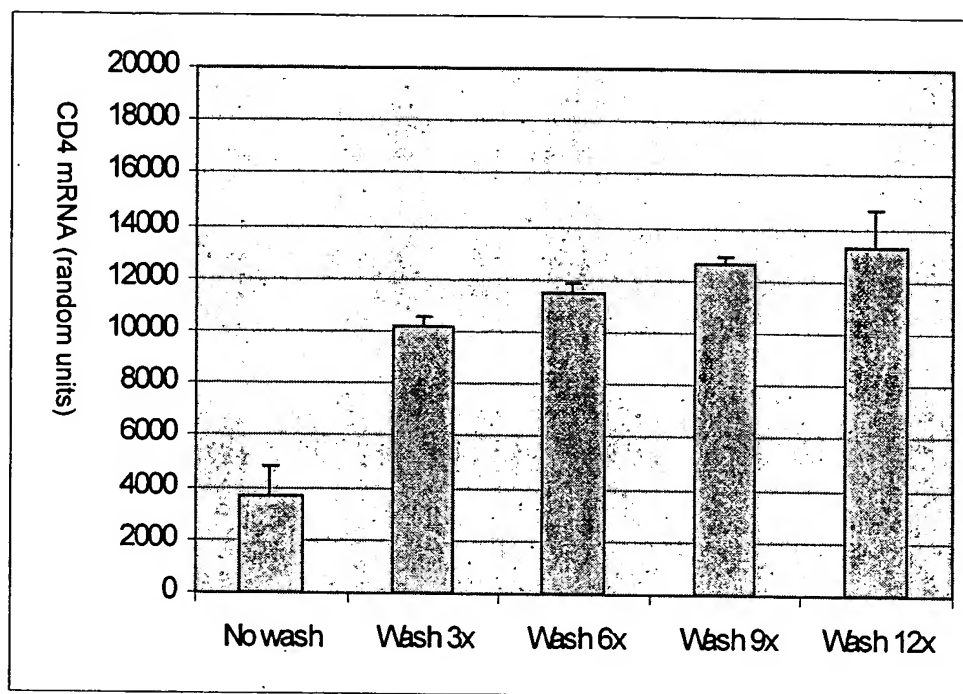


BEST AVAILABLE COPY

FIG 5. :

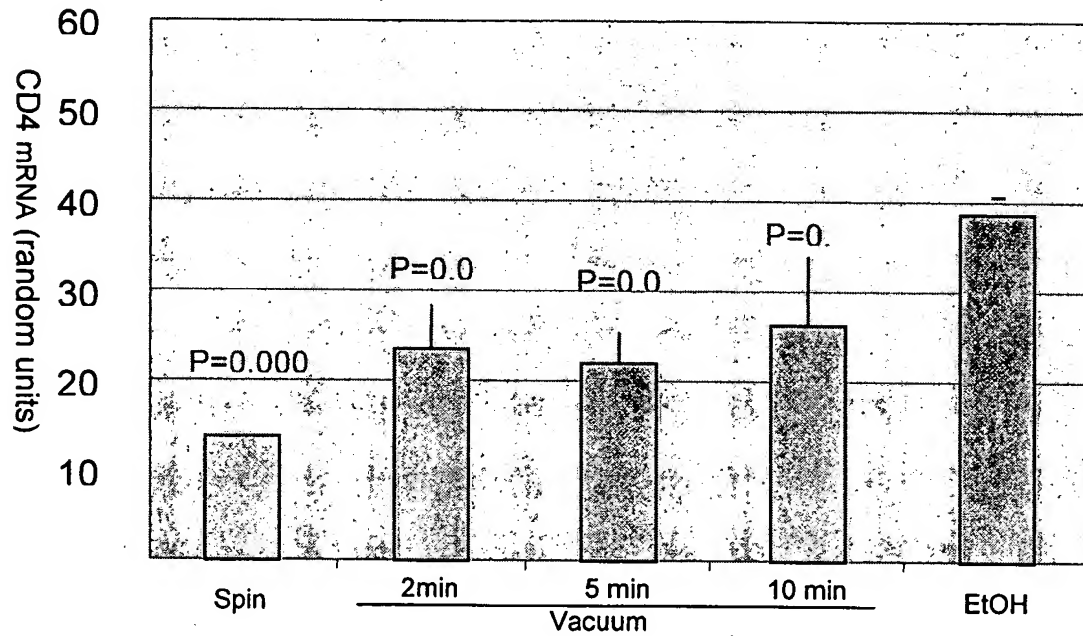

BEST AVAILABLE COPY


FIG 6.

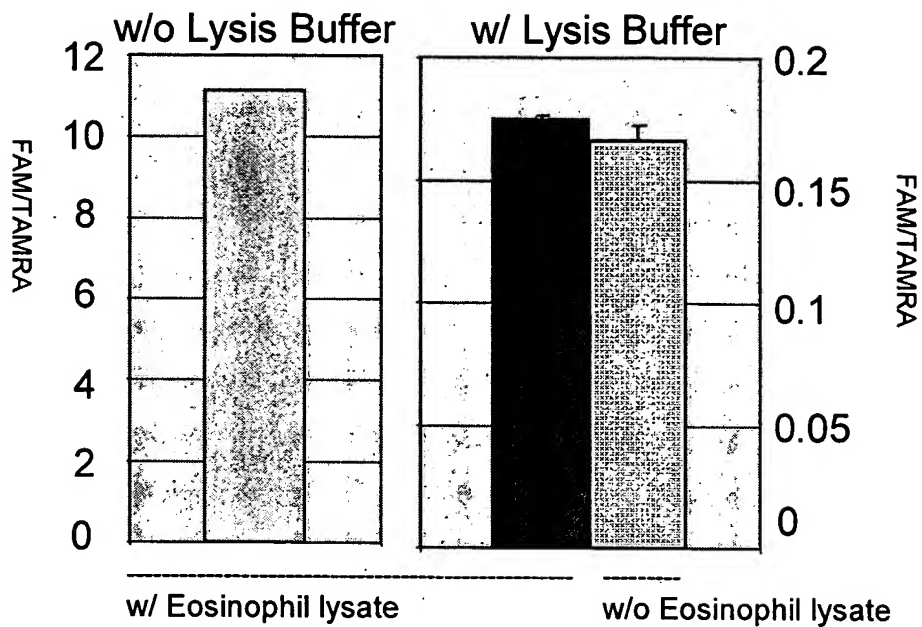

BEST AVAILABLE COPY


DEVICE AND METHOD FOR HIGH-THROUGHPUT  
QUANTIFICATION OF MRNA FROM WHOLE BLOOD  
Masato Mitsuhashi  
Appl. No.: Unknown Atty Docket: HITACHI.055CP1

FIG 7.

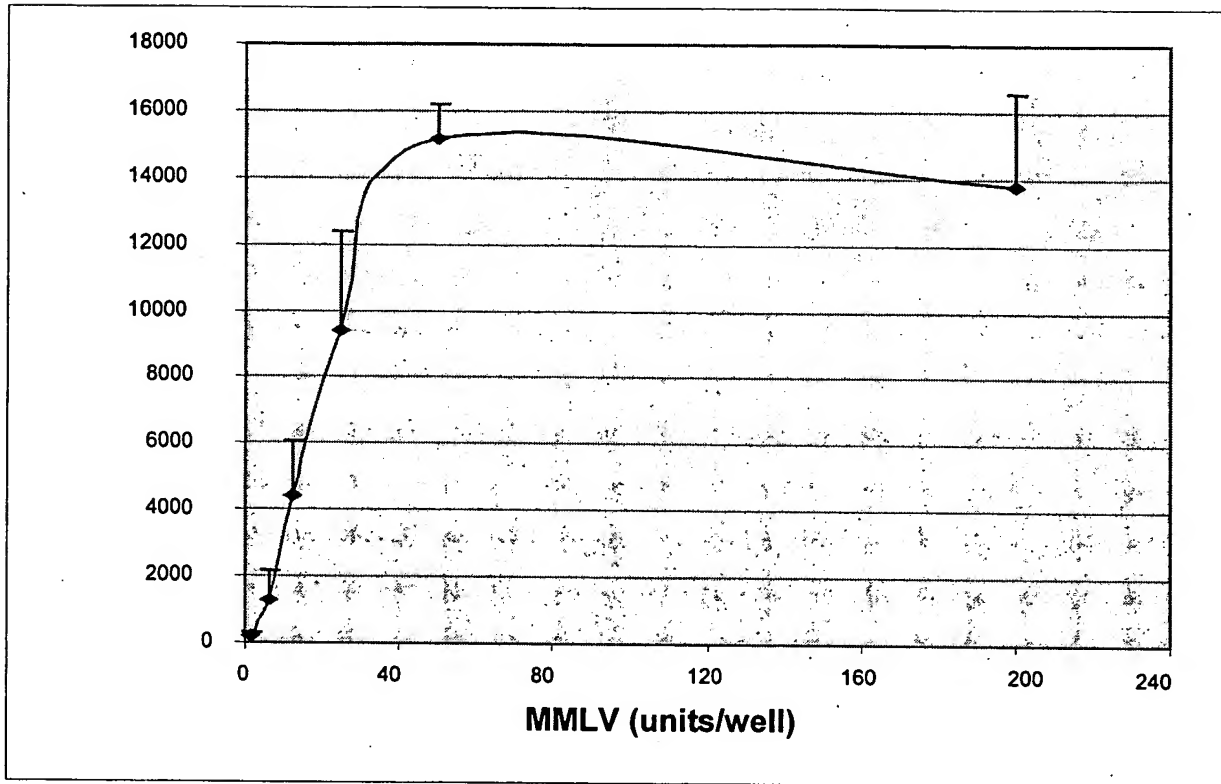

BEST AVAILABLE COPY

FIG 8.

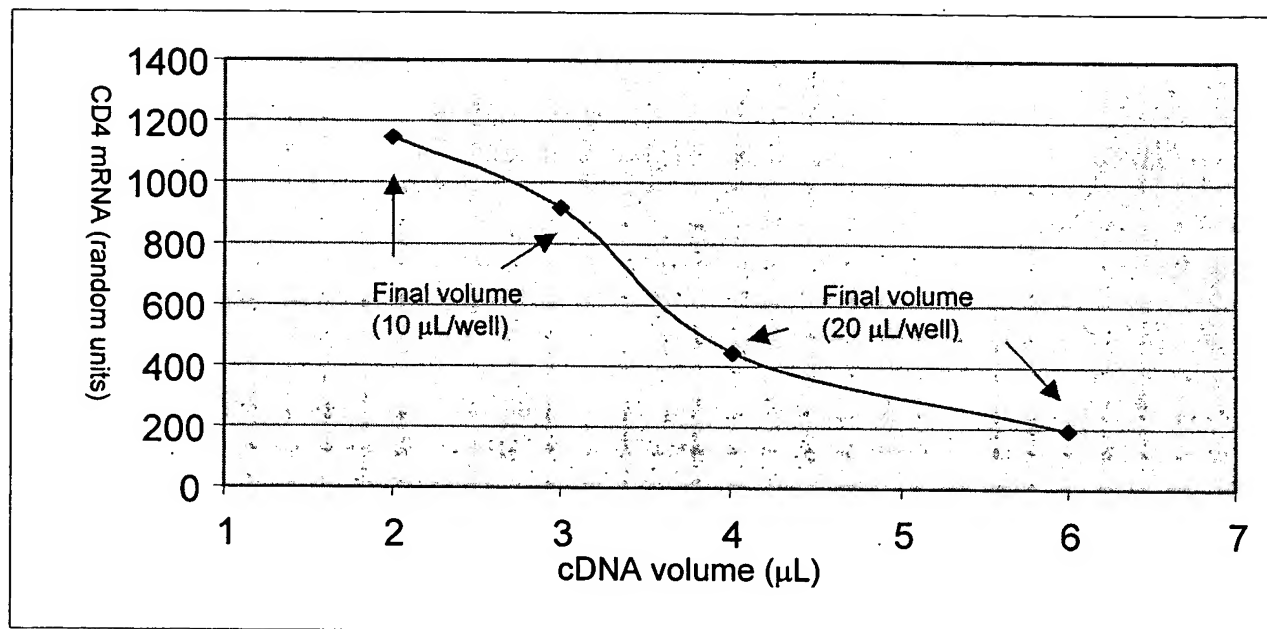

BEST AVAILABLE COPY




DEVICE AND METHOD FOR HIGH-THROUGHPUT  
QUANTIFICATION OF MRNA FROM WHOLE BLOOD

Masato Mitsuhashi

Appl. No.: Unknown


Atty Docket: HITACHI.055CP1

FIG 9.

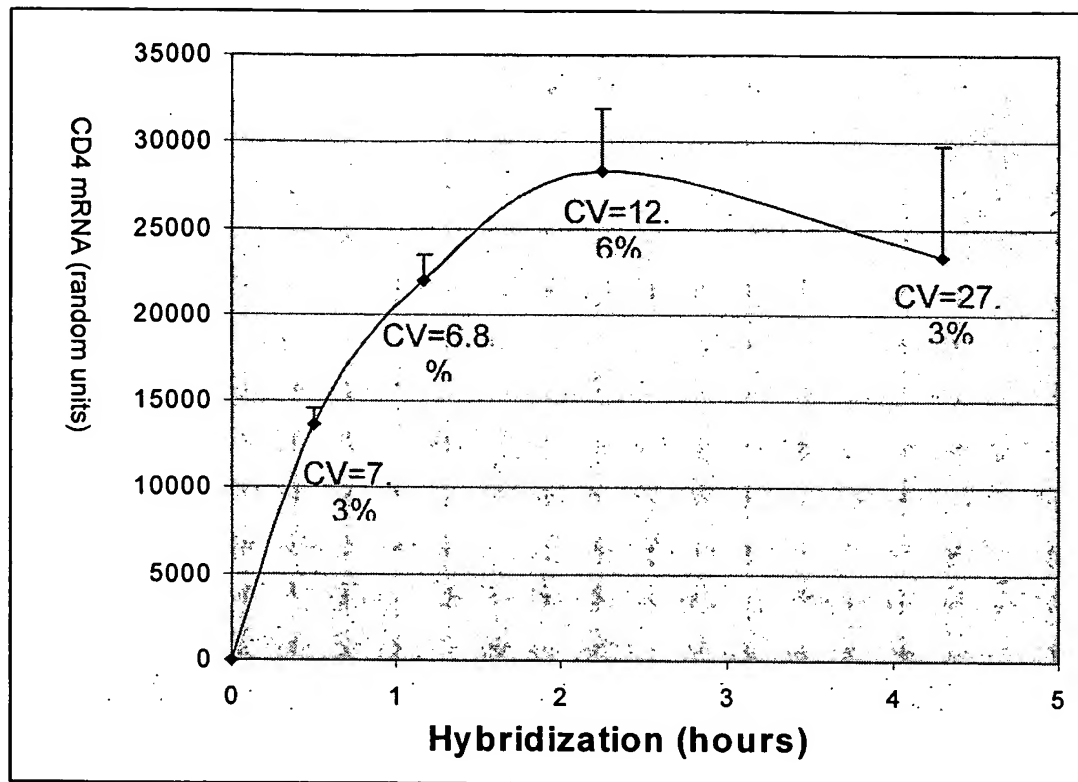

BEST AVAILABLE COPY

FIG 10.

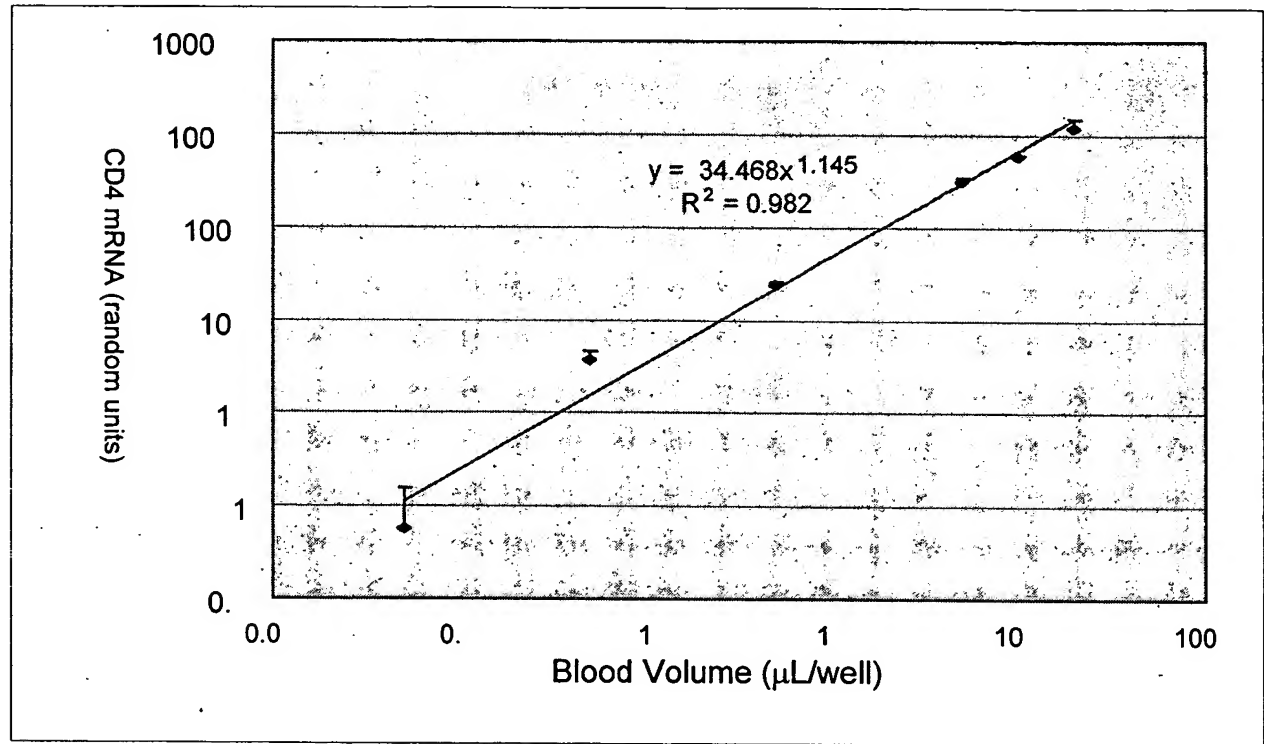


BEST AVAILABLE COPY

DEVICE AND METHOD FOR HIGH-THROUGHPUT  
QUANTIFICATION OF MRNA FROM WHOLE BLOOD

Masato Mitsuhashi

Appl. No.: Unknown Atty Docket: HITACHI.055CPI

FIG 11.

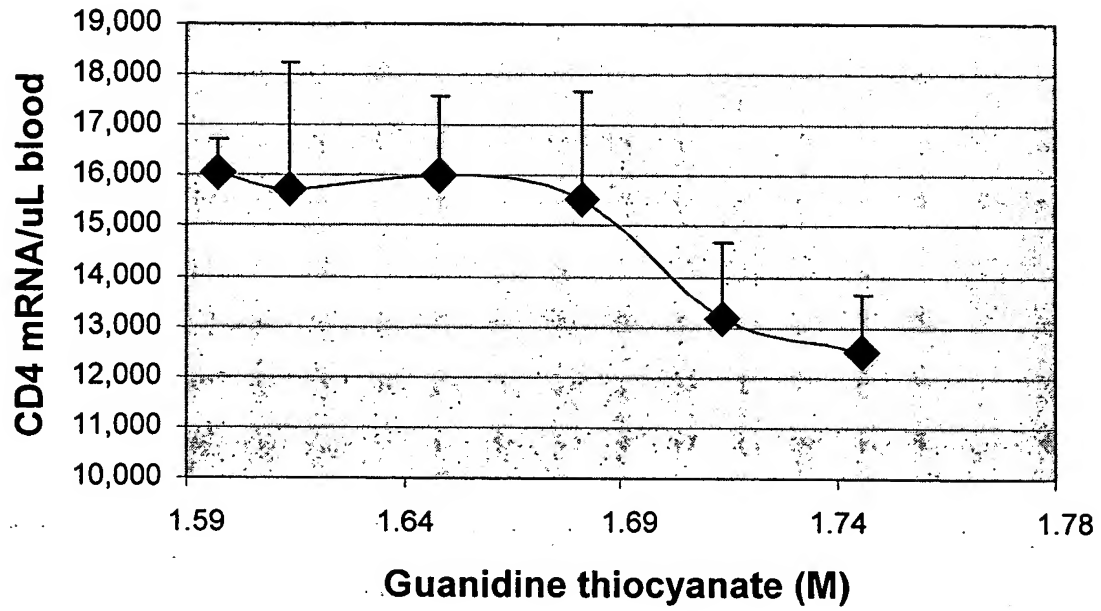


BEST AVAILABLE COPY

DEVICE AND METHOD FOR HIGH-THROUGHPUT  
QUANTIFICATION OF MRNA FROM WHOLE BLOOD

Masato Mitsuhashi

Appl. No.: Unknown Atty Docket: HITACHI.055CPI

FIG. 12.

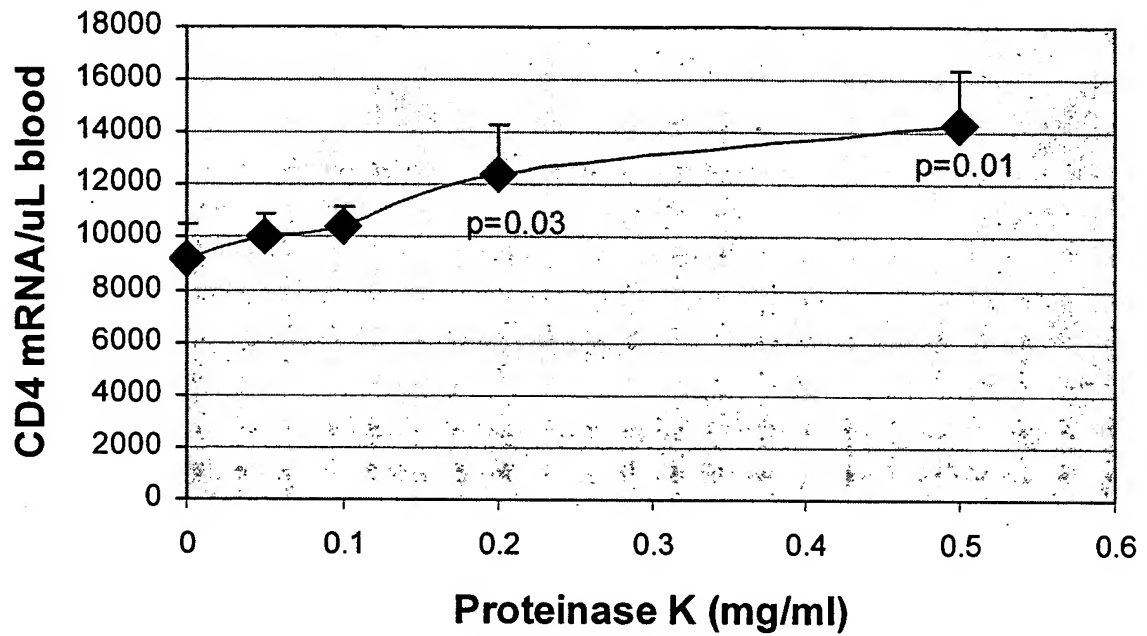

BEST AVAILABLE COPY